

# **OPTIFLEX**®

## **TABLE OF CONTENTS**

Precautionary Instructions
Foreword
Product Description
Package Contents
Installation
Operation Instructions
Quick Start
Pendant Functions
Other Pendant Functions
Pediatric Footplate Setup
User Maintenance
Technical Maintenance
Technical Specifications
Symbol Descriptions
Troubleshooting
Warranty
Parts Drawing
Parts List

## **PRECAUTIONARY INSTRUCTIONS**

**WARNING** – The following precautions should be taken in order to reduce the risk of fire, electrical shock, injury to persons or damage to the OptiFlex<sup>®</sup>:

- Read this manual before assembling or using OptiFlex.
- Only use OptiFlex on solid, flat surfaces.
- Extreme caution should be taken when in use around children.
- Use OptiFlex only as described in this manual.
- Keep hair, loose clothing, fingers and all parts of body away from moving parts of OptiFlex.
- DO NOT use OptiFlex outdoors or on wet surfaces.
- Materials may become flammable or combustible if exposed to a source of ignition.
- Disconnect electrical supply before servicing or cleaning. Failure to do so could result in electrical shock or personal injury.
- DO NOT use OptiFlex while smoking or around open flame.
- Exercise caution when using accessories and auxiliary devices such as muscle stimulators, ColPaCs and other modalities.
- Turn power off before unplugging.
- Unplug the power supply by grasping the plug not the cord.
- Damage may occur to OptiFlex if not transported and stored between 0 and 140°F (-18 to 60°C).
- Unplug from power supply when not in use.
- DO NOT use if cord or plug is damaged.
- Use extra care when touching metal of OptiFlex after exposure to cold or heat.
- DO NOT handle any electrical apparatus with wet hands.
- DO NOT use OptiFlex as a toy.
- Condensation could result and damage OptiFlex if unit is subjected to periods of low temperatures followed by periods of high temperatures.

- DO NOT use on unstable surfaces or liquid filled devices such as water mattresses or flotation pads.
- OptiFlex has been designed for maximum protection against the exposure of urinary incontinence. Precautionary measures should still be taken, though, when any type of liquid comes in contact with an electrical apparatus.
- OptiFlex is made from high impact materials. However, structural failure or hidden damage can be caused by shock, impact or dropping the unit. Use care when transporting and storing unit to avoid equipment damage.
- To isolate the unit from the power source, disconnect the power cord at the wall outlet.
- OptiFlex should only be used after the operator has thoroughly read and understands this manual.
- Rapid increases in ROM can cause complications.
- OptiFlex is not to be used in the presence of flammable anesthetic mixture with air or with oxygen or nitrous oxide.
- Meets IEC/EN 60601-1-2 Electromagnetic Compatibility/interference safety standard. (Care must be taken when operating this equipment around other equipment. Potential electromagnetic or other interference could occur to this or to the other equipment. Try to minimize this interference by not using other equipment in conjunction with it.)

## FOREWORD

This manual has been written for the owners and operators of the OptiFlex<sup>®</sup> continuous passive motion machine. It contains general instructions on operation, precautionary practices, maintenance and parts information. In order to maximize use, efficiency and the life of your OptiFlex, please read this manual thoroughly and become familiar with the controls as well as the accessories before operating the unit.

Specifications put forth in this manual were in effect at the time of publication. However, owing to Chattanooga Group's policy of continual improvement, changes to these specifications may be made at any time without obligation on the part of Chattanooga Group, Inc.

## **PRODUCT DESCRIPTION**

The OptiFlex is a continuous passive motion machine typically used postoperatively on total knee replacement and Anterior Cruciate Ligament (ACL) repair patients. By repeatedly flexing and extending the affected limb, the OptiFlex lessens the adverse effects of immobilization and trauma on the joint.

OptiFlex is a prescription device used under the supervision or by the order of a physician or other licensed healthcare provider.

## **PACKAGE CONTENTS**


- OptiFlex
- Control Pendant
- 1 Package of Soft Goods
- 1 Operator's Manual

## ! WARNING

- DO NOT plug in if switch is in ON position.
- DO NOT place leg in carriage until power is ON.
  If liquid or foreign object comes in contact with OptiFlex, turn power switch OFF and have authorized personnel check the unit.

## **CAUTION**

- Obese patients can suffer chafing due to contact with carriage frame.
- Failure to use securement strap correctly could change anatomical alignment resulting in tissue damage or joint injury.
- Unit must be placed on a solid, secure surface. Otherwise, unit could tip causing hip to be dislocated.









## INSTALLATION

OptiFlex<sup>®</sup> requires minimal installation. No lubrication is necessary and the unit is not required to be sterile.


- 1. Place OptiFlex unit on a solid, flat surface.
- 2. Attach the Soft Goods to the carriage of the OptiFlex by using the instructions provided with the Soft Goods.
- 3. Caution: Use only OptiFlex Soft Goods from the Chattanooga Group, Inc.
- 4. Plug the three-prong plug into a properly grounded wall outlet.

## **OPERATION INSTRUCTIONS**

Setup and operation of the OptiFlex is quick and easy. However, the operation instructions must be followed in order to ensure proper anatomical alignment and use of OptiFlex.

- 1. When setting up a new patient, activate RESET to clear the unit (see page 5). Measure the patient from hip joint (greater trochanter) to knee in centimeters. (Photo 1)
- 2. Adjust OptiFlex femur component to match hip to knee measurement in centimeters. (Photo 2)
- 3. Carefully place OptiFlex under the affected limb. Align knee joint with the corresponding hinge point on unit. (Photo 3)
- 4. Adjust the foot plate using the foot plate locking knobs so the patient's foot rests comfortably and the patient kit supports the leg from knee to foot. (Photo 4)
- 5. Secure the limb in the carriage frame by fastening the strap. (Photo 5)

### **QUICK START**

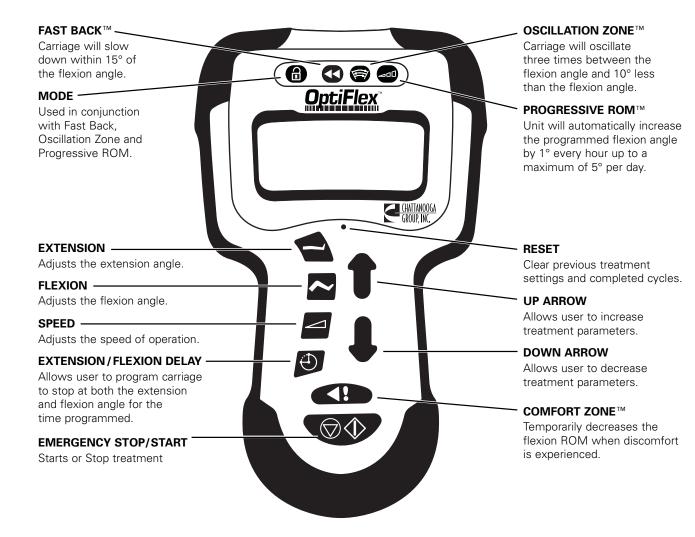

OPTIFLEX USER MANUAL

### **PENDANT FUNCTIONS**

All user input and feedback is provided through the pendant. The following are descriptions of each button provided with OptiFlex<sup>®</sup>.



Extension: View and modify the extension angle parameter.

*How to use:* To view the extension angle, press and hold the EXTENSION button. To modify the current extension angle, press and hold the EXTENSION button while pressing either the UP or DOWN ARROW.



Flexion: View and modify the flexion angle parameter.

*How to use:* To view the flexion angle, press and hold the FLEXION button. To modify the current flexion angle, press and hold the FLEXION button while pressing either the UP or DOWN ARROW.



**Speed:** View and modify the speed parameter.

*How to use:* To view the speed, press and hold the SPEED button. To modify the current speed, press and hold the SPEED button while pressing either the UP or DOWN ARROW.



**Extension/Flexion Delay:** View and modify the delay time for the extension or flexion angles. Using EXTENSION/FLEXION DELAY will cause the carriage to stop at the extension and flexion angle for the time programmed.

*How to use:* To view the extension/flexion delay time, press and hold the EXTENSION/FLEXION DELAY button. You can set independent DELAY times for extension and flexion. If an extension and or flexion delay time is required, simply hold down the DELAY button and the EXTENSION or FLEXION button and use the UP or DOWN ARROWS to adjust the time.

**Up Arrow:** Increases treatment parameters in conjunction with other buttons.

*How to use:* Select the specific function to increase (SPEED, EXTENSION, FLEXION or EXTENSION/FLEXION DELAY). While pressing and holding the appropriate button, use the UP ARROW to increase the value of the specified function.



**Down Arrow:** Decreases treatment parameters in conjunction with other buttons.

*How to use:* Select the specific function to increase (SPEED, EXTENSION, FLEXION or EXTENSION/FLEXION DELAY). While pressing and holding the appropriate button, use the DOWN ARROW to decrease the value of the specified function.



Reset: Resets all parameter and patient counters to factory defaults.

*How to Use:* To reset patient compliance counters, press and hold lightly by inserting a paper clip and accept reset by pressing the MODE button. To display total unit run time and cycles, press and hold RESET for 3 seconds, the total unit time and cycles are temporarily displayed.



**Emergency Stop/Start:** Starts or stops the treatment.

How to Use: Press the START/STOP button to begin or end the treatment.




**Comfort Zone**<sup>™</sup>: Temporarily decreases the flexion ROM when discomfort is experienced during treatment.

*How to Use:* Press and the carriage will immediately reverse direction to move toward the extension angle. For the next five cycles, the carriage will operate in a range five degrees less than the angle where the button was pressed. The Comfort Zone Flexion Angle is five degrees less than the angle where the button was pressed. Once five cycles are

### CAUTION – Emergency Stop/Start

When unit is stopped and STOP/START button is pressed, the unit will immediately begin moving in the opposite direction of the last movement.

#### COMFORT ZONE



- **C** = Comfort Zone activated temporary flexion limit established.
- $\mathbf{5^{o}}$  = Five degrees less than the angle where Comfort Zone was activated.

Upon completion of five cycles, ROM will increase by one degree each cycle until it reaches P.

- **P** = Programmed Flexion angle.
- **S** = Start/Finish.

## **!** WARNING

If pain is severe, do not use Comfort Zone. Stop treatment immediately. Failure to do so could result in tissue damage and could compromise surgical repair.

complete, the Comfort Zone<sup>™</sup> Flexion Angle will be increased by one degree each consecutive cycle until it reaches the currently Programmed Flexion Angle.

**Note:** If COMFORT ZONE is pressed within 30 degrees of the currently Programmed Extension Angle, treatment will stop and the message "Comfort Zone Too Small" will be displayed.



**Mode:** Used together with FAST BACK<sup>™</sup>, OSCILLATION ZONE<sup>™</sup> and PROGRESSIVE ROM button to enable and disable the appropriate mode. All three modes or any combination may be used at once.

*How to Use:* Press MODE button along with desired function (FAST BACK, OSCILLATION ZONE and/or PROGRESSIVE ROM).



**Fast Back<sup>™</sup>:** When the carriage reaches 15 degrees less than the Programmed Flexion Angle, it will begin to slow down. The deceleration rate will be half of the Programmed Speed when the carriage comes within 10 degrees of the flexion angle. Upon reaching the flexion angle, the carriage will reverse direction and resume the Programmed Speed as it moves towards the extension angle.

*How to Use:* While pressing and holding the MODE button, press the FAST BACK button to enable the FAST BACK mode

**Note:** If both FAST BACK and OSCILLATION ZONE modes are enabled, the carriage will move at the slower of 75°/min and half of the Programmed Speed while in the OSCILLATION ZONE ROM.

FAST BACK

Non-Working ROM	Working ROM (10°)
Fast Speed	Slow Speed
Fast Speed	Fast Speed
E	Working ROM Speed = 60°/min.
F = Programmed Flexion Angle	

**E** = Programmed Extension Angle



**Oscillation Zone™:** When the carriage reaches the Programmed Flexion Angle, it will oscillate between the Programmed Flexion Angle and ten degrees less than the flexion angle three times. The ten degree range of motion is known as the OSCILLATION ZONE ROM. While in the OSCILLATION ZONE ROM, the carriage will move at 75 deg/min or the Programmed Speed, whichever is slower. On the third oscillation cycle, the carriage will hold at the flexion angle for the Programmed EXTENSION/FLEXION Delay Time.

*How to Use:* While pressing and holding the MODE button, press the OSCILLATION ZONE button to enable the OSCILLATION ZONE mode.

**Note:** If both FAST BACK<sup>™</sup> and OSCILLATION ZONE modes are enabled, the carriage will move at the slower of 75 deg/min and half of the Programmed Speed while in the OSCILLATION ZONE ROM.




**Progressive ROM™:** When PROGRESSIVE ROM is activated, the unit will automatically increase the Programmed Flexion Angle by one degree every hour, up to a maximum of 5° per day.


*How to Use:* While pressing and holding the MODE button, press the PROGRESSIVE ROM button to enable the PROGRESSIVE ROM mode. Set the desired Final Flexion Angle by pressing and holding the FLEXION Button while using the UP and DOWN Arrows. Accept the Final Flexion Angle by pressing the MODE Button.

**Note:** The unit must run for a full hour at the entire ROM before the flexion angle will be increased. The unit will not automatically increase more than five degrees in any 24 hour period. Decreasing the flexion angle will automatically deactivate this mode.


#### **OSCILLATION ZONE**

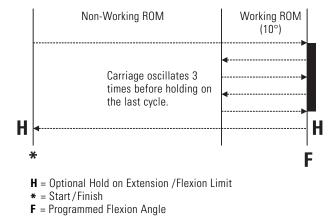

#### KNEE FLEXION ROM VS. TIME

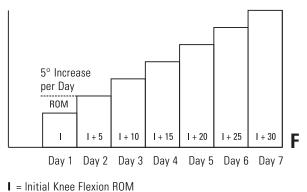

**F** = Final Knee Flexion ROM



### **OTHER PENDANT FUNCTIONS**

#### **Independent Delay Time**

You can set independent DELAY times for extension and flexion. If an extension and or flexion delay time is required, simply hold down the DELAY button and the EXTENSION or FLEXION button and use the UP or DOWN ARROWS to adjust the time.

#### **Selectable Scrolling**

The scrolling feature is disabled at the factory. Should you desire to enable this feature, simply press and hold the DELAY and MODE buttons. The display will scroll patient data for two (2) cycles then return to displaying Current Carriage Angle.

#### **Patient Lock-Out**

The Patient Lock-Out feature prevents the patient from changing any parameter except COMFORT ZONE<sup>™</sup> and START/STOP.

To enable the Patient Lock-Out feature: Press and hold the UP ARROW and the MODE button for three seconds. A single short beep will confirm that the feature has been activated.

Repeating the above sequence will deactivate the feature. A single short beep will confirm that the feature has been deactivated.

#### Language Selection

To select display language, press and hold the MODE and EXTENSION buttons simultaneously for 3 seconds. Use and arrows to select desired language and then press MODE to accept.

## **PEDIATRIC FOOTPLATE SETUP**

- 1. Remove footplate by loosening footplate knob.
- 2. Tighten flexion adjustment knobs.
- 3. Loosen the tibial adjustment knobs.
- 4. Remove footplate support.
- 5. Rotate 180 degrees and replace.
- 6. Rotate footplate frame 180 degrees.
- 7. Replace footplate.
- 8. Tighten all adjusting knobs.

## **USER MAINTENANCE**


To clean OptiFlex<sup>®</sup>, turn unit off and unplug the power supply. Clean OptiFlex with a damp cloth. DO NOT use abrasive cleaners. A small amount of mild household detergent may be used, if desired.

Soft Goods may be laundered as required. However, the same Soft Goods should not be used from patient to patient. Cleaning of Soft Goods will not meet the necessary sanitation guidelines. Replace Soft Goods for each patient.

## **TECHNICAL MAINTENANCE**

No attempt should be made to disassemble the unit. Maintenance and all repairs should be made by authorized personnel only.

The manufacturer will not be held responsible for the results of maintenance or repairs by unauthorized persons.

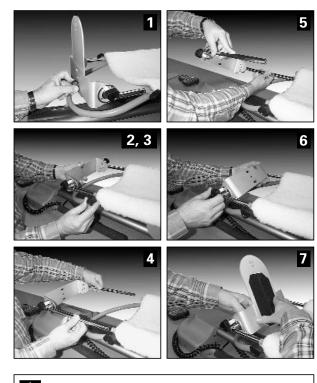



Disconnect electrical supply from outlet before servicing or cleaning the unit. Failure to do so could result in electrical shock.

## **TECHNICAL SPECIFICATIONS**

#### Safety

OptiFlex<sup>®</sup> complies with the following standards:

UL 2601-1

CAN/CSA 601.1

IEC/EN 60601-1

IEC/EN 60601-1-2

Meets MDD 93/42/EEC, CE 0413

Type "B" Equipment, Class I

Suitable for continuous operation

#### Unit


Input:	120 VAC~50/60 Hz, 40 Watts
Weight:	28 Lbs. (13 kg)
Length:	37 in. (94 cm)
Operation	
Knee Flexion ROM Limit:	120°
Knee Extension Limit:	10° Hyper Extension
Knee Speed Range :	30°/min. to 150°/min. Nominal
Maximum Patient Weight:	350 Lbs. (159kg.)
Calf Length Range: (knee joint to sole of foot)	10 to 23.5 in. (25.4 to 59.7 cm)
Thigh Length Range: (hip joint to knee joint)	12 to 19 in. (30.5 to 48.3 cm)

#### **Transportation and Storage**

Unit should be transported and stored within the following conditions:

Temperature:	0 - 140°F (32° - 60°C)
Humidity:	0 - 75% Relative Humidity


## **SYMBOL DEFINITION**







Start



Attention, Consult Accompanying Documents

## TROUBLESHOOTING

## ! WARNING

Disconnect electrical supply from outlet before servicing or cleaning the unit. Failure to do so could result in electrical shock.

The following is a solutions guide to minor performance problems. Only qualified personnel should service all other equipment problems.

PROBLEM	POSSIBLE CAUSE	POSSIBLE SOLUTION
OptiFlex® will not operate.	1. Unplugged at wall outlet.	1. Plug in and push ON/OFF button to ON.
	<ol> <li>2. ON/OFF button not turned ON.</li> <li>3. Power loss.</li> </ol>	<ol> <li>Push ON/OFF button to ON.</li> <li>Once power returns, unit will remain stopped until start button is pressed.</li> </ol>
	<ol> <li>Pendant unplugged.</li> <li>Carriage travel blocked.</li> </ol>	<ol> <li>Plug in pendant to unit.</li> <li>Unplug unit and remove obstruction from path of carriage.</li> </ol>
	6. Flexion angle set equal to extension angle.	6. Adjust extension angle smaller or flexion angle larger.
Treatment stopped in the middle of operation.	1. Motor overcurrent.	1. Press START/STOP button. Carriage will move in opposite direction.
	2. Comfort Zone too small.	<ol> <li>Comfort Zone button can only be used when ROM is greater than 30 degrees of Program- med Extension Angle.</li> </ol>

**Note:** Pendants of Optiflex<sup>®</sup> units model 2000 and 2020 will not function on Model 2030 and 2060 OptiFlex units.

### WARRANTY

#### **OptiFlex**

Chattanooga Group, Inc. ("Company") warrants that the OptiFlex<sup>®</sup> ("Product") is free of defects in material and workmanship. On the drive train components, including the motor, gearbox, drive screw, drive nut, shaft couple and all drive bearings, this warranty shall remain in effect for two (2) years. All other components shall be warranted for the amount of one (1) year from the date of original consumer purchase of this Product. This warranty extends to any owner of the Product during the warranty period. If this Product fails to function during the warranty period because of defect in material or workmanship, Company or the selling dealer will replace or repair this Product without charge within a period of 30 days from the date on which the defective Product is returned to the Company or the dealer. Company or the dealer will ship the replacement or the repaired Product to the consumer's facility.

All repairs must be performed by a service center authorized by Chattanooga Group, Inc. Any modifications or repairs performed by unauthorized centers or groups will void this warranty. To participate in warranty coverage, this Product's warranty registration card (included with Product) must be filled out and returned to Chattanooga Group, Inc. by the original owner within ten (10) business days of purchase.

#### Soft Goods Kit

Company warrants the Soft Goods Kit is free of defects in materials and workmanship. This warranty shall remain in effect for thirty (30) days.

#### **This Warranty Does Not Cover**

- 1. Replacement parts or labor furnished by anyone other than the Company, the dealer or an approved Company service agent.
- 2. Defects or damage caused by labor furnished by someone other than Company, the dealer or an approved Company service agent.

3. Any malfunction or failure in the Product while it is in the possession of the owner during the warranty period if the malfunction or failure is not caused by a defect in material or workmanship, or if the malfunction or failure is caused by unreasonable use, including the failure to provide reasonable and necessary maintenance.

#### Company Shall Not Be Liable for Incidental or Consequential Damages to Property or Business

Some states do not allow the exclusion or limitation of incidental or consequential damages, so the above limitation or exclusion may not apply to you.

TO OBTAIN SERVICE from Company or the selling dealer under this warranty, the owner must do or abide by the following:

1. A written claim must be made within the warranty period to the Company or the selling dealer. If the claim is made to the Company, written claim should be sent to:

4717 Adams Road P.O. Box 489 Hixson, TN 37343 USA Phone: 423-870-7200


2. The Product must be returned to the Company or the selling dealer by the owner.

This warranty gives you specific legal rights and you may also have other rights which vary from state to state.

The Company does not authorize any person or representative to create for it any other obligation or liability in connection with the sale of the Product. Any representation or agreement not contained in the warranty shall be void and of no effect.

## PARTS DRAWING

OPTIFLEX USER MANUAL

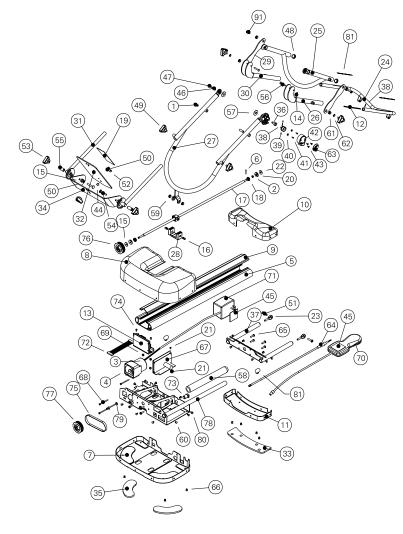

### **PARTS LIST**

ITEM NO.	ΩΤΥ.	PART NO.	ITEM NO.	ΩΤΥ.	PART NO.
1	2	J6028-BUSHING NYLON 5/16 OD	48	2	65991-TUBE PLUG
2	1	J1072-BUSHING NYLON 3/8 OD	49	4	J6012-KNOB MALE 1/4-20
3	1	40100-MOTOR BRUSHLESS	50	5	62066-SCREW 1/4-20x5/8
4	1	40101-GEAR BOX	51	2	J6052-SCREW 1/4-20x1
5	1	J2003-EXTRUSION	52	2 1	60396-SCREW 10-32x1/4
6	1	J6035-PIN COTTER	53	3	J6011-KNOB FEMALE
7	1	J2008-COVER REAR BOTTOM	53 4	2	
8	1	J2007-COVER REAR TOP	55		J6025-BOLT STOVE
9	2	J1025-WIPER	55 56	2	J6029-SPACER NYLON FOOT PLATE
10	1	J2005-COVER FRONT TOP	56	2	J6027-RIVET FEMUR HINGE
1	1	J2006-COVER FRONT BOTTOM	57	2	J6006-WASHER .312 IDx1 OD x .06
12	1	J1063-FEMUR BAR CATCH	58 59	1	68964-FOAM HANDLE GRIP
13	1	J6010-PCB MOTOR CONTROL		2	J6001-BEARING SPLIT FLANGE TRUNION
14	1		60	19	J6004-NYLON SNAP RIVET
15	4	87898-SPLIT PIN .125x3/4	61	4	J6005-BEARING SPLIT FLANGE PIVOT
16	2	J6044-WASHER .252x.62x.06 THK.	62	2	J6051-SNAP RING
17	1	J1055-PIN TRUNION	63	1	J1050-DECAL POT
18	2	J2004-ACME ROD	64	1	J6040-CABLE KNEE POT
19		J6008-BEARING FLANGE	65	8	J6000-SCREW SELF TAP 10-24
20	.14 YD. 2	J1067-VELCRO HOOK	66	9	66058-RIVET
20	3	COUCH BEAMING HOLLEH	67	1	J6043-PCB MAIN
21	1	71319-SCREW 6-32×1/4	68	4	J6048-SCREW 8-32x2 SOC HD
22	2	J6034-WASHER FLAT BEARING	69	4	21733-NUT 8-32 ESNA
	2	J6020-ROD END PLT'D	70	1	J2022-PENDANT S/A
24		J1014-FEMUR SUB ASSY	71	1	J6056-POWER SUPPLY
25	1 1	J1022-THIGH S/A	72	1	J6042-MOTOR CONTROLLER CABLE
26		J1026-FEMUR HINGE LF.	73	1	J2023-CABLE PENDANTRECEPTICAL
27	1	J1011-CALF S/A	74	2	70099-SCREW 6-32x3/8
28	1	J1034-SLIDER	75	1	J2000-DRIVE BELT
29	2	J1032-FEMUR LINKAGE	76	1	J2001-PULLEY BALL SCREW
30	1	J1030-FEMUR HINGE RT.	77	1	J2002-PULLEY MOTOR
31	2	J1036-FOOT ROD S/A	78	1	J2009-BASE REAR S/A
32	1	J2014-FOOT PLATE	79	2	70105-WASHER #10 FLAT
33	1	J1058-PAD FRONT	80	2	53793-SCREW #10x1/2 PAN TEK
34	1	J2013-FOOT PLATE FORMED	81	2	J6065-HEYCO RT ANG STRAIN RELIEF
35	2	J1057-PAD REAR			
36	1	J1041-PIN POT PIVOT			
37	1	J1075-BASE FRONT S/A	NOTE 1		SUPPLY FOR J2015, OPTIFLEX 120V CPM
38	2	J6023-SPLIT PIN 1/16x9/16			IOWN IN EXPLODED DRAWING
39	.021	J6002-TUBE POT PIN	131/143	0050. 51	IOWIN IN EXI LODED DIAWING
40	2	J6003-SERVO MOUNT CLEAT			FOR J2019. OPTIFLEX 220V CPM
41	2	J6002-SCREW #4-40			DITIONAL CORD SET IS NEEDED
42	1	J1003-COVER POT			. (NOT SHOWN )
43	3	J6024-SCREW POT MOUNT 6-32	101122		. (NOT SHOWIN)
44	1	J1071-PIN FOOT ROTATION			
45	.11YD.	J1068-VELCRO LOOP			
46	1	J1061-SLEEVE CARRIAGE PIVOT			
47	1	J6007-SCREW PIVOT 1/4-28x5/8			

## More Trusted Products from Chattanooga Group, Inc.

**Achiever**<sup>™</sup> Supports **Adapta**® Treatment Tables A.E.R. Boot® Auto Edema Reduction Boot AirMedex ™ Alternating Pressure Mattress boo-boo pac™ Child Size Bear-Shaped Cold Pack Cambion® Shock Dampening Foot Care Products Carpal-Trac™ Carpal Traction Accessory ColPaC® Chilling Units and Reusable Cold Therapy Products Conductor Gel<sup>™</sup> Highly Conductive Ultrasound Gel **Contracture Products** Contracture Management Orthotic Products CTS ™ Carpal Tunnel Stretching Device Dura-Stick™ Electrodes Self-Adhesive Electrodes EMG Retrainer® Dual Channel Surface EMG **ErgoWave**® Intersegmental Traction Table Flexi-Pac® I and II Reusable Hot and Cold Compresses Gel Medex™ Gel Mattress Overlay Hydrocollator® Heating Units and HotPacs™ **Hydrogel**® Conductive Gelpad Dressings Intelect<sup>®</sup> Legend Ultrasound and Electrotherapy Products

Measurement Instruments Dynamometers, Goniometers, etc. Myossage<sup>®</sup> Massage Lotion Nvlatex® Elastic Wraps Optiflex® Continuous Passive Motion PALS<sup>™</sup> Electrodes Neurostimulation Electrodes Para-Care® Paraffin Wax Unit Pillow Perfect™ Cervical Pillow Line Pivotal Therapy System™ Orthotics for the Spine ProPower Pillow™ Power Massage Pillow PresSsion® Intermittent Compression Pron Pillo® Positioning Pillow **Cervical Traction System Clinical Cervical Traction** SPORT-PAC<sup>™</sup> Soccer Ball Shaped Cold Pack Therma-Wrap™ Hot and Cold Compression Triton® Treatment and Traction Equipment TX® Treatment and Traction Equipment Vectra™ Series Ultrasound and Electrotherapy products. Wellness 1st™ Back Support Women's Contour Back Support

Back Support

The first real innovation in CPM in a decade!



**ISO 9001 CERTIFIED** 

4717 Adams Road P.O. Box 489 Hixson, TN 37343 u.s.a. 1-423-870-2281 1-800-592-7329 u.s.a. 1-800-361-6661 canada + 423-870-7200 INTERNATIONAL + 423-870-2046 INTL. FAX www.chattgroup.com

**((** 0413

J2021B

© 2000 Chattanooga Group, Inc.